




IFA

Institut für Arbeitsschutz der
Deutschen Gesetzlichen Unfallversicherung

CHECK x **5**

FAULTLESS MASKS?

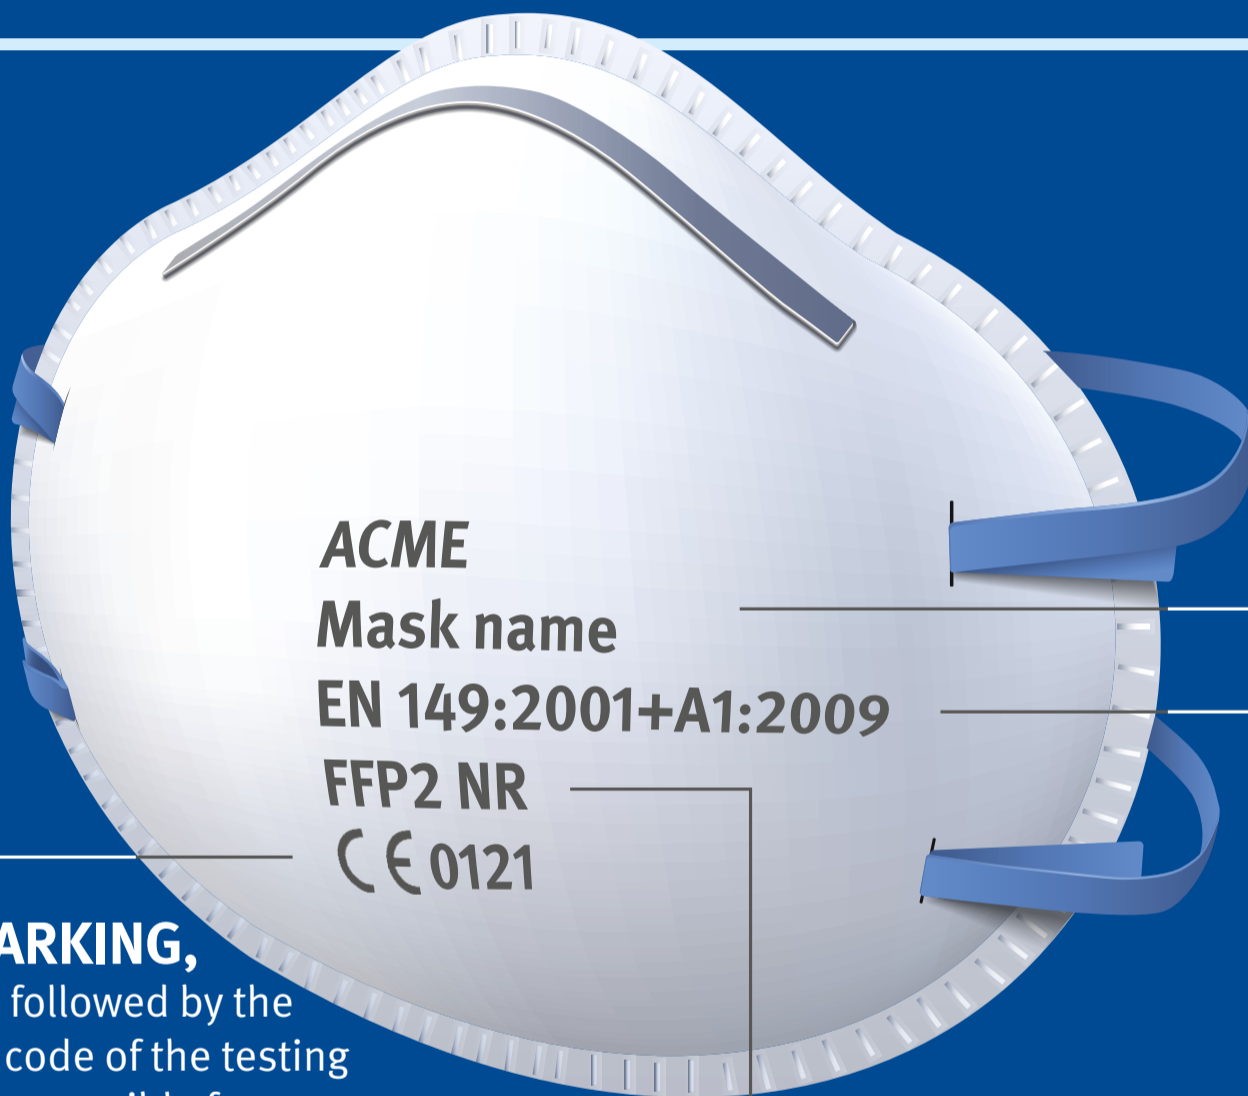

1 CE MARKING,
always followed by the
4-digit code of the testing
body responsible for
surveillance
(0121 = IFA). Is the testing
body authorized to test
respiratory protective
devices?

2 CHECK online:
TESTING BODY
correct?



3 CLASS: FFP1, FFP2 or FFP3,
followed by a space;
suffix (mandatory): NR = non-reusable after one shift;
R = reusable;
suffix (optional): D (suitable for high dust levels)

5 COMPANY NAME
or other reference to
manufacturer;
PRODUCT NAME

4 Number and year of
publication of
**EUROPEAN TESTING
STANDARD**

If these **5** criteria are **NOT** met,
the mask is **NOT** a type FFP
respiratory mask tested in
compliance with the standards.